

UP: 1408
DOB: 16-Jun-1963
57yr, Male


Benny Smith

Vent rate: 60 BPM
PR int: 241 ms
QRS dur: 100 ms
QT/QTc: 415/416 ms
P-R-T axes: -1 39 35

ABNORMAL ECG

UNCONFIRMED REPORT

3/24/2021
J. Houston
MD

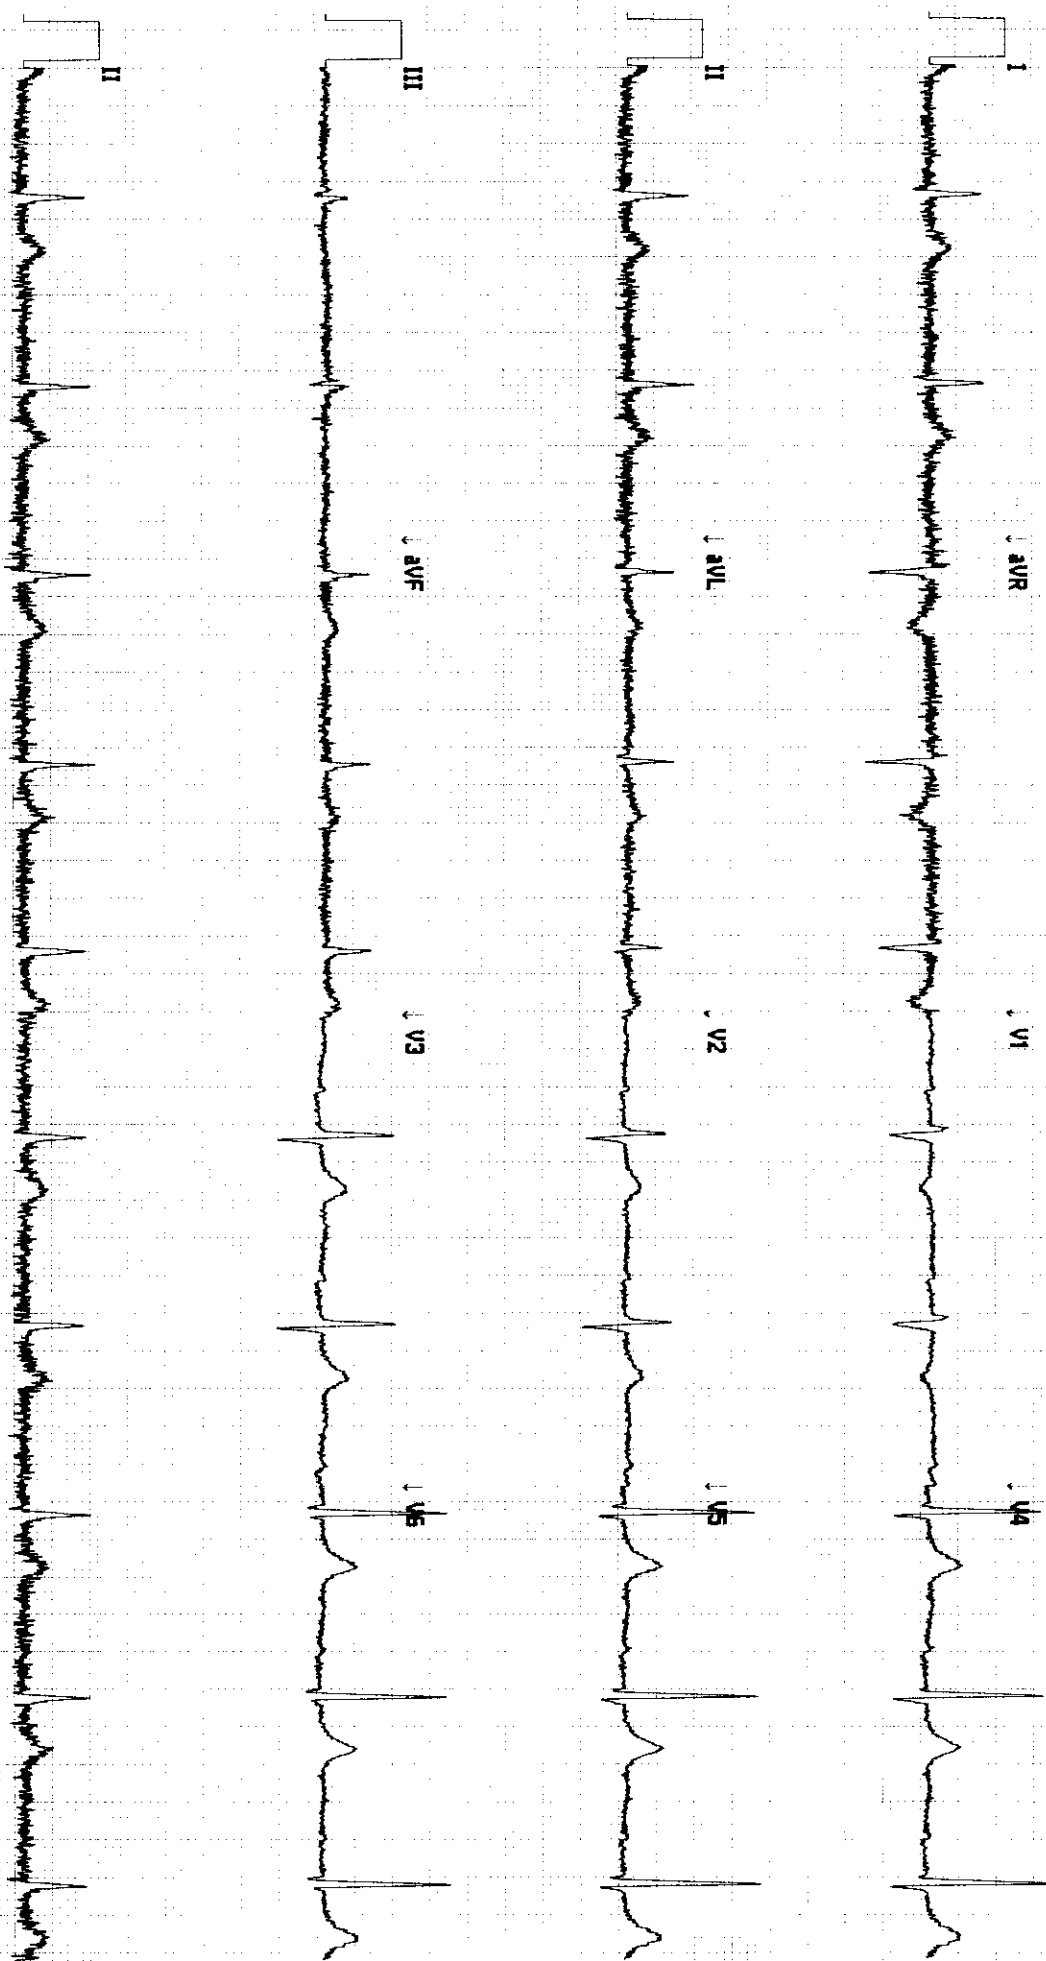

116190431764

No Site Name

Site: 0 Cart * 0 Version 2.10.5 Sequence #00296 25mm/s 10mm/mV 0.05-150 Hz
Welder/Allyn